

# FILLING PATTERN MEASUREMENT USING A 500 MHZ DIGITIZER AT SOLEIL AND APS STORAGE RINGS

D. Bisiach, M. Cargnelutti, P. Leban, M. Žnidarčič, Instrumentation Technologies doo, Solkan, Slovenia  
N. Hubert, D. Pedeau, SOLEIL, Gif-sur-Yvette, Paris, France  
A. Brill, N. Sereno, ANL, Lemont-Illinois, USA

## ABSTRACT

Filling pattern was measured at SOLEIL and APS storage ring using a 500 MHz digitizer. Various filling patterns were measured: from a single bunch to a multi-bunch hybrid fill. The digitizer has 14-bit granularity and locks the sampling clock to exact RF frequency (352 MHz). Signals were sampled from the standard BPM pickup and APD diode. Data were retrieved using Matlab and Labview interfaces and compared to existing systems.

## INTRODUCTION

An essential part of the synchrotron diagnostics system involves the investigation of the bucket distribution during the operation.

Modern light sources allow to operate with different filling pattern modes (e.g. single bunch, multi-bunch, hybrid patterns), and knowledge of the real-time bunch charge longitudinal distribution can help to tune the beam stability and performance [1].

Digitizers with high ADC resolution and wide dynamic range are an alternative to the existing high sampling rate oscilloscopes that are commonly used in combination with BPM pick-up or APD diode detectors.

The Libera Digit 500 is a 500 MHz/14-bit ADC digitizer based on the CavityBPM hardware [2] with the possibility to customize the frontend (e.g. input bandwidth, additional filters...).

The purpose of these measurements was to confirm that the Libera Digit 500 could be used as a filling pattern monitoring device in case of BPM pickups and to evaluate its behavior also using diode detectors [3].

## MEASUREMENTS - SOLEIL

The fill pattern monitoring testing consisted of testing two setups, the first using a BPM pickup as a bunch detector and the second using an APD diode setup.

### Fill pattern monitoring using BPM

The original filling pattern monitoring instrumentation at Soleil consists of an Agilent Digitizer with 8 GS/s-8 bit resolution.

The setup with the Libera Digit 500 AC was implemented to retrieve the signal directly from a pickup using attenuators and phase shifters to tune the signal delays and the bunch flat top.

The pickup outputs (A, B, C, and D) were connected to fixed attenuators. Each attenuator output entered a mechanical phase shifter. Since the signal power was still too high some additional attenuators were placed before the signal splitter-combiner. The combined signal then entered an additional mechanical phase shifter.

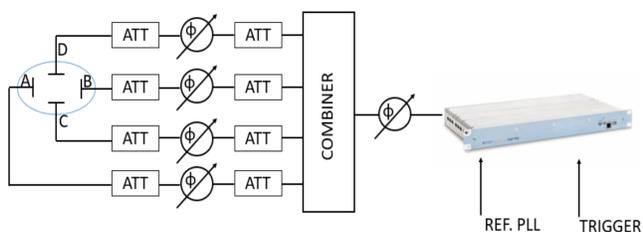


Figure 1 – Instrument setup with BPM

Every single channel delay was set equal with the first mechanical phase shifter (maximizing each signal amplitude having the three other channels disconnected). This trick allows us to set the same time delay on all the 4 channels, resulting in a sync sum signal from the pickup to the Libera Digit 500.

Once all the 4 channels had the same time delay set the second mechanical phase shifter was used to reach the maximum signal amplitude which assured the sampling point to be on the flat top of the measured pulse.

The signal from the BPM was tested with different filling patterns and at different currents: single bunch, 8 bunches, and 1 quarter filling.

The signal level was adjusted with the frontend attenuators.

The length of the acquisition buffer was 650000 data points which correspond to 1562 turns. The acquisition noise is pretty constant over the input scale.

During the 8 bunches machine operation mode, the flat top acquisition point was shifted in the slope direction reaching the 75% and 50% of the original maximum amplitude, RMS noise did not increase.

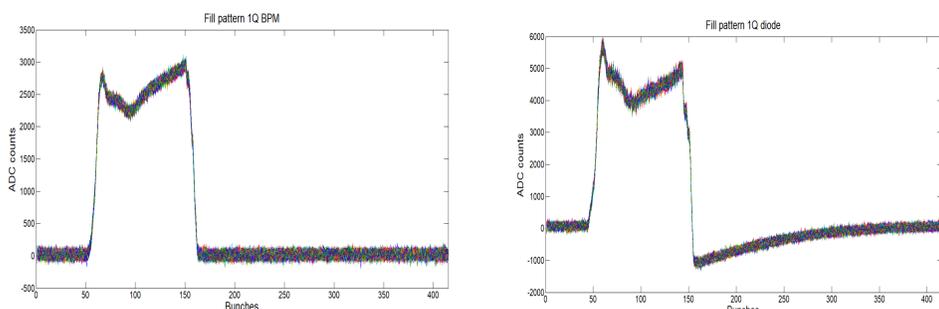


Figure 2 – 1Q filling pattern. On left signal from BPM, on right signal from APD diode

The AC Libera Digit500 gives identical results in term of resolution compared to the initial SOLEIL setup on a BPM signal and is an appropriate system for filling pattern monitoring on such signal.

### Fill pattern monitoring using APD diode

The Libera Digit 500 was connected to an existing set-up using an APD diode. The original setup was monitoring the signal with an oscilloscope (an Agilent Digitizer with 8 GS/s-8 bit resolution, 1 GHz bandpass frequency).

The Libera Digit 500 was connected to the diode output. The measurement with the diode is more delicate because its linearity range is too small to cover the current full scale. We kept the diode output amplitude constant at ~0.3 V adjusting for each current optical densities at the input. With 21 dB attenuation in the Libera Digit 500, it corresponds to ~7000 counts on the ADCs.

The effect of the AC coupling on the Libera Digit 500 can be seen and consists in a recovery effect due to the DC component (which was not present on the BPM set-up), this is reported for a one quarter filling on Figure 2.

## MEASUREMENTS - APS

The BCM used for the reference measurement is a Xilinx FPGA-based device developed by the Advanced Light Source (ALS). It uses a Virtex-6 FPGA, with an FMC104 14-bit 250MSPS ADC. Interleaved sampling is used to obtain 46 sample points per bucket, and 1024 turns are averaged to determine the charge for each bunch. An EPICS IOC converts ADC counts into bunch current using the SR DCCT value. The Libera Digit500 was connected to a spare set of bpm buttons. These bpm cables were connected directly to the buttons and phase-matched with mechanical phase shifters, and then combined with a combiner (500-5000 MHz). An attenuator was used on the combined signal to bring the output signal to a safe range for the Digit500 input. The input RF clock phase was adjusted with phase shifters to maximize the ADC counts of the signal of the Digit500. For the 'scaled' plot, the BCM units were in mA (positive peaks), while the Digit500 units were ADC counts (negative peaks). The mean of each was calculated to find the scaling factor to plot them both together.

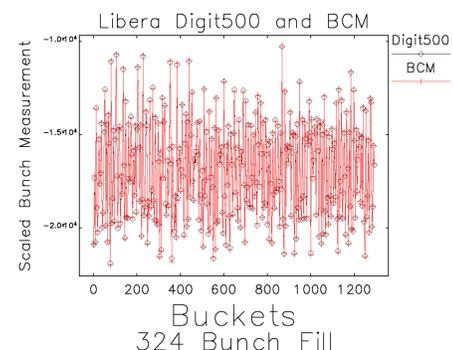


Figure 3 – A 324 bunch fill pattern comparison between Libera Digit 500 and the existing BCM

Figure 3 reports a comparison between the Libera Digit500 and the existing BCM device. The storage ring was filled with 324 bunches.

It is possible to see that the peaks corresponding to the BCM readout (in red) are well aligned with the peaks detected by the Libera Digit 500 (grey dots).

## CONCLUSIONS

The performed measurements proved the capability of the Libera Digit 500 to perform as an efficient fill pattern monitoring system for light source storage rings.

The module works perfectly for acquiring the BPM signal. This behavior is supported by the results from both testings at SOLEIL and APS storage ring.

When connected to the photodiode detector the AC coupling distorts the signal due to the DC component coming from the diode.

## ACKNOWLEDGEMENTS

The authors are grateful to SOLEIL and APS storage rings for providing a testbench for various measurements.

## REFERENCES

- [1] C. Y. Wu, J. Chen, K. T. Hsu, K. H. Hu, and C. H. Kuo, "Fill-ing Pattern Measurement for the Taiwan Light Source", in Proc. 11th European Particle Accelerator Conf. (EPAC'08), Genoa, Italy, Jun. 2008, paper TUPC038, pp. 1137-1139.
- [2] M. Cargnelutti et al., "Design and Simulations of the Cavity BPM Readout Electronics for the ELI-NP Gamma Beam Sys-tem", in Proc. 7th Int. Particle Accelerator Conf. (IPAC'16), Busan, Korea, May 2016, pp. 264-266. doi:10.18429/JA-CoW-IPAC2016-MOPMR017
- [3] P. Leban, S. Bassanese, G. Brajnik, and R. De Monte, "Eval-uation of a New 500 MHz Digitizer at Elettra and Fermi", in Proc. 10th Int. Particle Accelerator Conf. (IPAC'19), Mel-bourne, Australia, May 2019, pp. 2635-2637. doi:10.18429/JACoW-IPAC2019-WEPGW071